





Serinus[®] 60

Nitrogen Dioxide Analyser with CAPStechnology

USEPAdesignated equivalent method — Cavity Attenuated Phase Shift (CAPS)—allows direct measurement of nitrogen dioxide (NO₂), rather than an indirect calculation from a chemiluminesc ence analyser.

No converter, no high vacuum, no ozone and no chemical reactions are required.

The Acoem Serinus 60^{*} is an affordable NO₂ analyser that gives accurate and timely results.

* Acoem Serinus 60 formerly known as Ecotech Serinus 60.

acoem.com

Serinus 60 Theory of Operation

The measurement of nitrogen dioxide (NO_2) utilises Cavity Attenuated Phase Shift (CAPS)spectroscopy technology. sample air is filtered to remove particulates and dried before entering the precision stainless steel 264 mm measurement cell.


The measurement cell contains two high reflectivity mirrors located at either end to provide an average optical path length of several kilometres. A modulated blue light source emits a narrow band wavelength of 450 nm which is used as a photon source for the cavity attenuation process. The LEDis pulsed into the optical cavity and the photon 'leakage', as a result of the optical cavity, is determined through the output voltage measured by the vacuum photodiode detector. The detector is used in conjunction with a narrow band-pass interference filter (450 nm).

During LED modulation the photon leakage of the cavity combined with photon absorption from gas molecules within the cavity produces a shift in the phase of the response signal measured by the detector.

By measuring the shift in phase angle without NO_2 in the sample (background) a baseline phase shift can be measured. During operation, NO_2 gas molecules within the cavity will increase photon decay and this will be reflected as a change in phase of the detector signal. This change in phase is proportional to the NO_2 concentration. Using this principle it is possible to reliably measure NO_2 concentrations of well under 1ppb up to 1000 ppb. Due to the continuous measurement of the sample, the analyser has a fast response time of less than 30 seconds.

Approvals


• USEPAdesignated equivalent method

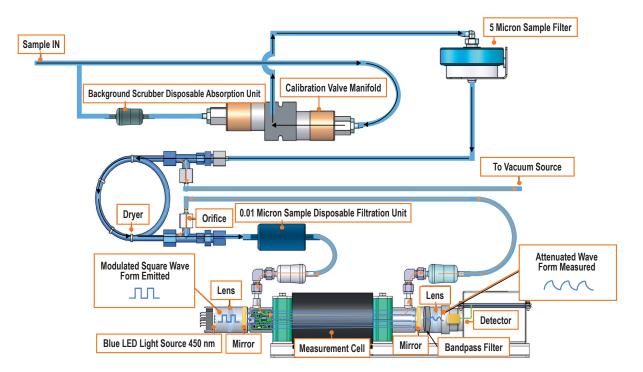



Specifications

Ranges:	0 - 1ppm
Concentration display:	mg/m³, µg/m³, ppm, ppb or ppt
Noise:	< 0.02 ppb
Lower detectable limit:	0.04 ppb or 0.5 %of reading, whichever is greater
Linearity:	1%to < 400 ppb
	4%to full scale
Precision:	0.04 ppb or 0.5 % of reading, whichever is greater
Zero drift:	< 0.75 ppb
Span drift:	< 1.5ppb or 0.5 %of reading, whichever is greater
Response time:	< 30 seconds
STPreference:	0 °C,20 °C,25 °C at 101.3 kPa
Sample flow rate:	500 cc/min
Temperature range:	0 - 45 °C
Operating Voltage:	100 - 240 VAC,50 - 60 Hz (autoranging)
Power Consumption:	88 VA(typical at start up)
	65 VA(after warm up)
Dimensions:	429 x 175x 638 mm
Rack Spacing:	3.5 RU
Weight:	19.4 kg

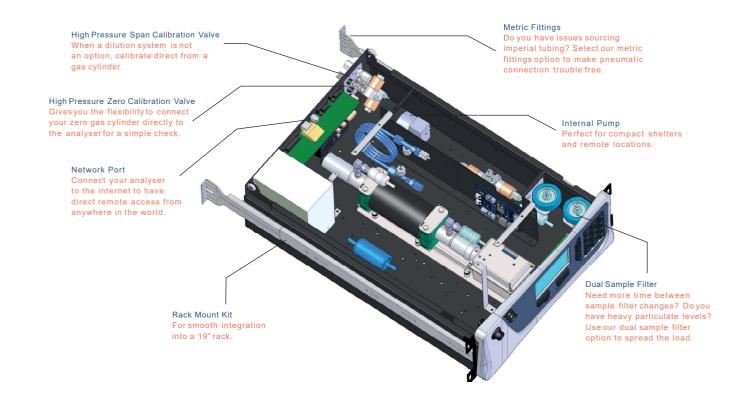



Communication

- •USBport (digital communication)
- •Bluetooth* (digital communication via Android App)
- •TCP/IPEthernet network connection*
- RS232 Port 1: Digital communication
- RS232 Port 2: Multidrop port
- Protocols: Modbus RTU/TCP,Bayern-Hessen, EC9800, Advanced.

Inputs / Outputs

- •25 pin I/O port
- Menu selectable current output of
- 0 20, 2 20 or 4 20 mA
- Menu selectable voltage output of 0 to 5 V or 0 - 10 V, with offset of 0 V, 0.25 V or 0.5 V
- Autorangingfrom 0 50 ppb to 0 100 ppm
- •3 scalable analog inputs, 0 5 V, 160 µV resolution
- 8 logic level digital status inputs/8 open collector digital outputs.

Data logging

- 8 GBremovable USBflash memory drive that stores the internal data logger, event log, automatic/manual configuration backup & automatic/manual parameter listsave
- Internal data logger (can log up to 12 of 200+ parameters)
- Data logger interval from 1 second up to 24 hours user selectable
- Storage capacity of ~10years at a 1 minute interval.





* Optional.

Specifications subject to change without notice. Images used are for illustrativepurposes only. Alltrademarks and registered trademarks are the property of their respective owners.

 $\ensuremath{\textcircled{\sc 0}}$ 2022 Acoem and all related entities. All rights reserved. 20221212

acoem.com

Official Distributor

XEARPRO Via delle Primule, 16 Cogliate (MB) - 20815, Italia info@xearpro.com

└ +39 02 9646.0317
□ xearpro.it